

Pilot clinical study of quantitative ultrasound spectroscopy measurements of erythrocyte aggregation within superficial veins

Boris Chayer^a, Louise Allard^a, Zhao Qin^a, Julian Garcia-Duitama^{a,b}, Laurence Roger^a, François Destrempe^a, Jean-François Cailhier^c, André Denault^d and Guy Cloutier^{a,b,e,*}

^aLaboratory of Biorheology and Medical Ultrasonics, University of Montreal Hospital Research Center (CRCHUM), Montréal, QC, Canada

^bInstitute of Biomedical Engineering, University of Montreal, Montréal, QC, Canada

^cCRCHUM and Department of Medicine, University of Montreal, Montréal, QC, Canada

^dMontreal Heart Institute, University of Montreal Hospital, and Department of Anesthesiology, University of Montreal, Montréal, QC, Canada

^eDepartment of Radiology, Radio-Oncology and Nuclear Medicine, University of Montreal, Montreal, QC, Canada

Abstract.

BACKGROUND: An enhanced inflammatory response is a trigger to the production of blood macromolecules involved in abnormally high levels of erythrocyte aggregation.

OBJECTIVE: This study aimed at demonstrating for the first time the clinical feasibility of a non-invasive ultrasound-based erythrocyte aggregation quantitative measurement method for potential application in critical care medicine.

METHODS: Erythrocyte aggregation was evaluated using modeling of the backscatter coefficient with the Structure Factor Size and Attenuation Estimator (SFSAE). SFSAE spectral parameters W (packing factor) and D (mean aggregate diameter) were measured within the antebraial vein of the forearm and tibial vein of the leg in 50 healthy participants at natural flow and reduced flow controlled by a pressurized bracelet. Blood samples were also collected to measure erythrocyte aggregation *ex vivo* with an erythroaggregometer (parameter S_{10}).

RESULTS: W and D *in vivo* measurements were positively correlated with the *ex vivo* S_{10} index for both measurement sites and shear rates (correlations between 0.35–0.81, $p < 0.05$). Measurement at low shear rate was found to increase the sensitivity and reliability of this non-invasive measurement method.

CONCLUSIONS: We behold that the SFSAE method presents systemic measures of the erythrocyte aggregation level, since results on upper and lower limbs were highly correlated.

Keywords: Erythrocyte aggregation, quantitative ultrasound, shear rate control, human, clinical measurements

*Corresponding author: Dr Guy Cloutier, Laboratory of Biorheology and Medical Ultrasonics, University of Montreal Hospital Research Center (CRCHUM), Montréal, Québec H2X 0A9, Canada. Tel.: +1 514 890 8000/Ext. 24703; E-mail: guy.cloutier@umontreal.ca.

30 1. Introduction

31 Since there is no clinical way to monitor acute inflammation on the bedside, blood biomarkers
32 (mainly cytokines and plasma proteins) remain the only available indicators of severe inflammation
33 leading to possible hypotension and sepsis [1]. However, these biomarkers are not amenable to follow
34 progression of the acute inflammatory response in critically ill patients due to the requirement of
35 repeated blood sampling and delay in receiving these laboratory measures. There is thus a need for
36 inflammation monitoring, as this condition may be reversed with appropriate timely treatment [2].

37 Inflammation modulates the level of red blood cell (RBC) aggregation. Erythrocytes, which natu-
38 rally tend to form rouleaux-type structures, do form, however, more compact clump-type aggregates,
39 whenever inflammatory plasma molecules and conditions affecting their cellular membrane's proper-
40 ties are present [3–5]. It has long been demonstrated that ultrasound is sensitive to the presence of RBC
41 aggregation and that the backscattered signal from flowing blood is enhanced with the aggregate size
42 [6–9]. Quantitative ultrasound (QUS) methods are nowadays well known for their ability to provide
43 non-invasive information on tissue microstructures [10]. Among QUS approaches, modeling of the
44 backscatter coefficient with a spectral descriptor has been widely applied to various organ tissues. The
45 structure factor size and attenuation estimator (SFSAE) was specifically developed to analyze a dense
46 medium such as blood constituted by a high volume concentration of acoustic scatterers [11, 12]. An *in*
47 *vivo* proof-of-concept using the SFSAE model of the backscatter coefficient was reported on diabetic
48 patients with poor metabolic control [13]. Recently, Garcia-Duitama et al. [14] proposed a protocol to
49 insure reproducibility of backscatter ultrasound measurements of RBC aggregation and demonstrated
50 the need for controlling the venous flow to maintain a low shear rate condition.

51 In this study, we aimed at exploring different strategies that would be compatible with ultrasound
52 measurements in critical care units. Measures were repeated to evaluate the robustness of proposed
53 methods. Our hypothesis is that it is possible to acquire ultrasound data at the bedside using a bracelet
54 positioned over the vein of interest to control the flow, and an ultrasound device and a post-processing
55 computer algorithm to measure RBC aggregation based on the SFSAE model.

56 2. Materials and methods

57 2.1. Outlines

58 For this pilot clinical evaluation, healthy volunteers were selected and measurements were repeated
59 to evaluate the intra-subject variability. A homemade bracelet to control the blood flow was designed
60 (Fig. 1), and a computer platform to monitor measurements was developed. The monitoring system
61 allows a user to visualize the B-mode ultrasound image of the vein and to record radiofrequency
62 (RF) data. RF images are then processed using a particle image velocimetry algorithm to measure the
63 maximum blood velocity so as to provide feedback to the user for adjusting the pressure applied by
64 the bracelet over the vein to reduce the blood flow. Acquired RF data at a predetermined low shear rate
65 and under natural flow were used to measure RBC aggregate structural parameters with the SFSAE
66 algorithm. Measurements were performed on two vascular sites that would be accessible for patient
67 monitoring.

68 2.2. Subject recruitment and protocol

69 After approval by the Ethics Committee of the Centre Hospitalier de l'Université de Montréal
70 (CHUM) and having obtained signed informed consents, fifty participants (25 men and 25 women)

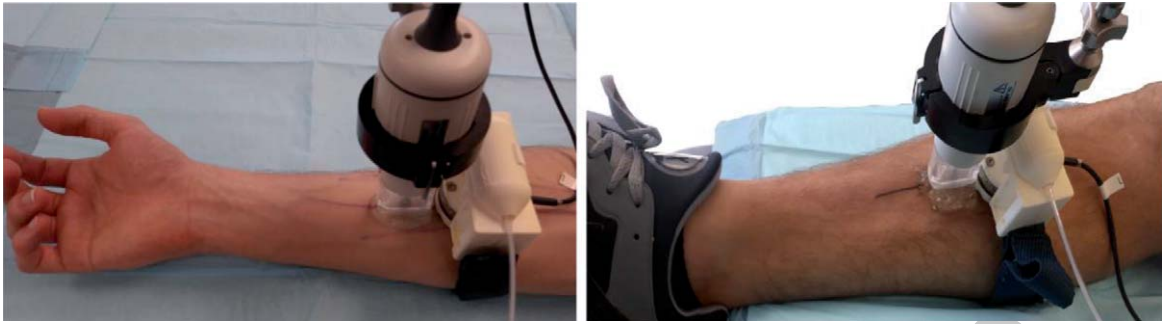


Fig. 1. Picture showing the load cell mounted on the pneumatic bracelet device, the venous architecture of the forearm and leg marked with ink, and the Visualsonics ultrasound probe RMV-703 positioned over the region of the measure.

71 were enrolled in this pilot study. Men and women were aged 43.9 ± 19.4 and 46.7 ± 18.6 years old,
 72 and their body mass indices (BMI) were 24.3 ± 4.4 and 25.1 ± 3.1 , respectively. This cohort involved
 73 European (43), Asian (4) and North-African ancestries (3) participants. Some of them self-reported
 74 having at least one of the following chronic disease conditions: type 2 diabetes (3), lupus (1), aortic
 75 aneurysm (1), high cholesterol (9) and hypertension (5). Participants were lying down on an exam bed
 76 and ultrasound data were acquired on the palmer side of the forearm on the antebrachial vein, and on
 77 the tibial vein on the front of the leg. Ultrasound acquisitions were performed with a high-frequency
 78 scanner (Vevo770, 35 MHz central frequency probe #RMV-703, Visualsonics, Toronto, Canada). For
 79 each measurement site, veins with a diameter larger than 1 mm were quested to facilitate ultrasound
 80 post-processing. After the ultrasound probe was set in place with a rigid stand, a B-mode image was
 81 acquired to measure the vein depth, which corresponds to the span between the skin surface and the
 82 closer vessel wall. The internal vein diameter was also measured in this manner before each assessment
 83 of RBC aggregation.

84 2.3. Low shear rate acquisition procedure using the designed bracelet

85 As introduced earlier, a homemade pneumatic compression bracelet (Fig. 1) was designed to apply
 86 a smooth pressure on the skin over the vein for regulating the flow and reducing the shear rate into
 87 the blood vessel. This was based on Garcia-Duitama et al. experiments [14] that have shown that
 88 keeping a pre-measuring low residual venous shear rate enables reproducible *in vivo* RBC aggregation
 89 measurements. The bracelet was positioned 10 mm downstream to the ultrasound acquisition site. After
 90 positioning the ultrasound probe, the blood flow was initially stopped by inflating the pneumatic device
 91 and then released to validate that the bracelet could control the blood flow. The compression bracelet
 92 included an embedded load cell (mini40, ATI Industrial Automation, Apex NC., USA) allowing real-
 93 time measurement of the force applied on the skin. The load cell controller was calibrated and sent
 94 the applied force [in Newton] through a RS232 communication directly to a Matlab program (version
 95 2014a, Natick, Ma, USA) every second. Five ultrasound measurements were made with and without
 96 the flow controlling bracelet to measure the intra-subject variability, so as to reach low shear rate
 97 and natural shear rate conditions, respectively. An infrared instrument was used prior to ultrasound
 98 probe and bracelet positioning to facilitate the identification of the venous architecture (model AV400,
 99 AccuVein, Huntington, NY, USA). With a non-permanent pen, the vasculature was mapped on the
 100 surface of the skin and a straight venous segment without major bifurcations within a distance of at
 101 least 40 mm was selected. When such a vein segment was not available (17 cases for the leg and one
 102 for the forearm), only measurements without bracelet were performed (i.e., natural flow).

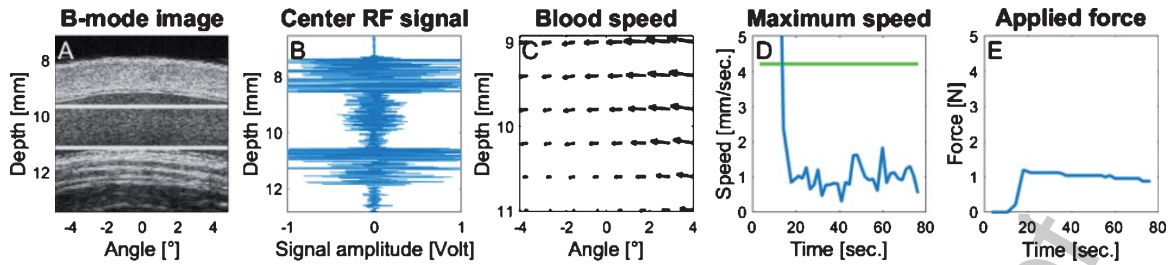


Fig. 2. Illustration of the control panel used during data acquisition. Each panel was automatically refreshed over time. (A) Longitudinal B-mode image of the vein; (B) acquired radiofrequency ultrasound data (depth versus normalized amplitude); (C) displacement map of the blood flow, the length of each vector corresponds to the instant displacement. The blood speed map region corresponds to the region delimited by the 2 white horizontal lines within the flow stream of panel A. (D) Maximum flow velocity within the blood speed map over time (in mm/s versus s), the green line corresponds to the threshold limit according to the vein diameter; (E) force applied by the bracelet and monitored by the force sensor over time (in Newton versus s).

Acquired RF echoes were amplified (model 5900PR, Panametrics inc, Waltham, Ma, USA) and recorded using a 12-bit 250 MHz digitizer (GageScope 12501, Dynamic Signals LLC, Lockport, IL, USA) at a frame rate of 26 per second. A computer platform interface (Fig. 2), developed in Matlab, allowed monitoring the blood flow velocity within the vein (Fig. 2D), and the pressure applied by the bracelet (Fig. 2E). The blood flow velocity was computed using a particle image velocimetry (PIV) algorithm [15] applied on RF blood signals. The maximum velocity in the central portion of the vein (horizontal lines in Fig. 2A) was determined every second and used to manually control the pressure into the bracelet. The RF data quality control (Fig. 2B) displayed an A-line at the center of the B-mode image to validate that no saturation occurred in the blood signal (data clipping would affect the computation of the backscatter coefficient). The B-mode quality control (Fig. 2A) displayed the central position of the vein that was adjusted to match the transducer focus depth at 10 mm, thus ensuring an optimum signal-to-noise ratio.

During bracelet inflated pressure adjustment, the maximum blood velocity was monitored instead of the mean shear rate for convenience purpose. Indeed, instead of computing the shear rate from PIV data using the spatial derivative of the velocity field, which would require a real-time vessel wall segmentation to determine the vein boundary, it was determined experimentally that a low residual shear rate condition could be fulfilled if the maximum speed remained close to 1 mm/sec. This method was suitable for most participants, even those with very small venous flow. For every measurement, the bracelet pressure was gradually increased until the maximum blood velocity into the vein reached 1 mm/s (Fig. 2D). When the optimum pressure allowing the targeted maximum speed was attained (Fig. 2E), one minute was allowed prior to RF ultrasound data acquisition to ensure a stabilized RBC aggregation condition. Then, the bracelet pressure was released and one minute was left between every repeated acquisition.

2.4. Natural shear rate measurements

Natural shear rate measurements were made after controlled flow acquisitions; whenever applicable, the ultrasound probe was left in place to maintain the same recording site within the vein. The protocol for natural flow acquisitions was the same as described above. The bracelet was deflated and left in place. A one minute waiting period was left between every repeated acquisition. Because the natural blood flow velocity produced PIV aliased measures (velocity too high considering the frame rate), the

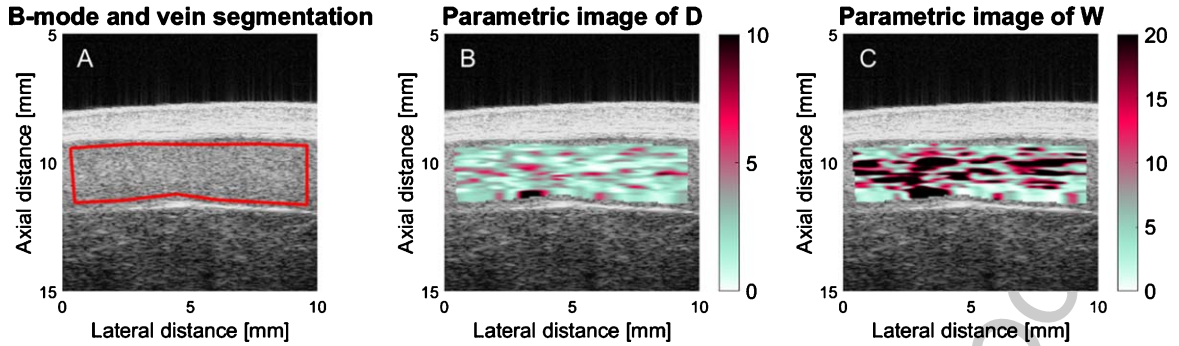


Fig. 3. B-mode (A) and parametric images of D and W (B and C, respectively) computed for the segmented region (red boundaries in A) of the vessel lumen of patient ID number 29. D is the mean RBC aggregate diameter and W is the packing factor. Regions close to the vessel wall are intentionally not selected to compute the backscatter coefficient only for blood flow signals. Black areas in B and C correspond to missing information due to a poor correlation between the backscatter coefficient and the SFSAE spectral model.

maximum blood velocity was assessed using power Doppler ultrasound after the last acquisition of repeated measurements.

2.5. Backscatter coefficient assessment and SFSAE modeling

Details on QUS SFSAE estimation can be found elsewhere [16]. A fourth-order Butterworth band-pass filter (15–37 MHz) was first applied on RF signals. Then, a region of interest (ROI) was manually delineated within the central region of the vein lumen (Fig. 3A). To avoid computing SFSAE values with RF data corresponding to the vessel wall, the segmentation was made to reject signals too close (less than 64 samples) to the vessel boundary. The ROI was then partitioned into resolution cells of 5 scanlines laterally, each comprising 128 samples axially with 50% overlap.

The mean experimental backscatter coefficient as a function of frequency was computed for every resolution cell, and averaged in the time-domain over 20 consecutive images prior to processing the SFSAE method. In order to compensate for instrument dependent signal conditioning, the reference backscatter coefficient method was used [17]. Two parameters of the SFSAE method were computed: D and W (Fig. 3B, C). D represents the mean diameter of aggregates (expressed in RBCs diameter assuming isotropic clustering). W corresponds to the packing factor (dimensionless), which describes the compactness of aggregates. Both D and W parameters increase with the enhancement of RBC aggregation. Based on simulations [18], it was demonstrated that $W = C_1 \times D^2 + C_2$, where constants C_1 and C_2 are close to 1.0 and 0.0, respectively. Values of these constants are influenced by the hematocrit that is an input parameter of the SFSAE model. The blood hematocrit of each participant was measured by micro centrifugation.

To filter outliers in parametric images of D (Fig. 3B) and W (Fig. 3C), SFSAE spectral models from resolution cells providing poor fits with experimental backscatter coefficients were rejected (*i.e.*, if the correlation R^2 within the frequency bandwidth of 15–37 MHz was below 0.5, see [19]). To extract a representative value of the aggregation state, median values of D and W were computed within the segmented venous ROI. The median was then averaged over 5 repeated measurements, prior to computation of correlations with other parameters (see below).

2.6. *Ex vivo* assessment of RBC aggregation

A 4 mL blood sample was taken less than 2 hours before or after US examination for all participants. Blood hematocrit was adjusted to 40% with autologous plasma and processed in an erythroaggregometer (Regulest, Florange, France). The aggregation index at 10 sec (S_{10}) was computed, which is a dimensionless parameter proportional to the RBC aggregation kinetics [20]. This measure corresponds to the relative surface under the reflected laser backscatter curve during the first 10 sec after applying a high shear rate to disaggregate RBCs. This value was used as a gold standard reference to compare with the proposed ultrasound method for assessing the systemic RBC aggregation level of flowing blood.

2.7. *Data reporting and statistical analysis*

The SFSAE D and W parameters are presented as mean \pm standard deviation (SD) computed over all measurements for a given configuration. The reliability of the SFSAE method was assessed by computing the intraclass correlation coefficient (ICC) between 5 repetitive measurements. The ICC and its 95% confidence interval were computed using R statistical software (version 3.2.5, R Foundation, Vienna, Austria). An ICC between 0.75 and 0.9 corresponds to a good reliability, whereas a value between 0.5 and 0.75 indicates moderate reliability [21]. Spearman correlation was computed between D, W, and *ex vivo* S_{10} measurements, since these parameters vary non-linearly as a function of erythrocyte aggregation. To verify the potential influence of gender on values of D, W and S_{10} , Student *t*-tests were used. The mean intra-subject variability was calculated as the variance divided by the mean of the 5 repeated measurements and averaged over all participants. Repeated ANOVA (RANOVA) tests were performed to evaluate any relationship between the 5 repeated SFSAE measures and the measurement order, and any relationship between the force applied and the measurement order. The median shear rate within the selected vein was estimated by substitution of the measured maximum velocity and vessel diameter into the Ostwald-De Waele power law model [22]. See Appendix 1 for a mathematical description of this model.

3. Results

This protocol required acquisition of 1000 ultrasound datasets (50 patients, two recording sites, two flow conditions, five repetitive measurements). However, as given in Table 1, only 760 RF acquisitions could be performed. In the forearm, the vessel size was too small (1 person) or a collateral vein was too close to the measurement location, thus preventing a stable shear rate condition at low flow (1 person). Over the leg, we observed more tortuosity of the tibial vessel and shorter segments length without collateral veins. Moreover, the measurement with a bracelet was more complicated over the ankle due to its curvature because the footprint of the pneumatic occluder was designed to apply a force perpendicular to the limb. Consequently, 36 individuals over 50 could be studied over the leg at natural flow, and 19 at reduced flow.

3.1. *Adjustment of the applied force to reduce the flow*

The force applied by the pneumatic occluder to reduce the flow within the brachial vein of the forearm was quite small at 1.5 ± 1.2 N (Table 1). Over the leg, the required force to adjust the flow was slightly higher at 2.7 ± 1.9 N. Figure 4 reports the applied force on the forearm for every subject. For a single participant, the required force was similar along the 5 measurements (mean intra-subject

Table 1

Technical parameters associated with the ultrasound acquisition protocol for two locations (forearm and leg) and two blood flow conditions (one requiring a bracelet to apply a compression on the vein, the other at natural flow)

	Forearm with bracelet	Forearm natural flow	Leg with bracelet	Leg natural flow
Number of measurements	48	49	19	36
Bracelet applied force	1.5 ± 1.2 N	–	2.7 ± 1.9 N	–
Maximum blood velocity	0.6 ± 0.3 mm / s	28 ± 2 mm / s	0.6 ± 0.4 mm / s	28.2 ± 3.2 mm / s
Estimated shear rate	0.8 ± 0.2 s ⁻¹	37.8 ± 22.3 s ⁻¹	0.7 ± 0.3 s ⁻¹	37.4 ± 38.2 s ⁻¹
Coefficient of variation of the shear rate	30%	59%	38%	102%
Deepness of the vein	1.8 ± 0.8 mm		1.9 ± 0.5 mm	
Diameter of the vein	1.5 ± 0.4 mm	1.4 ± 0.4 mm	1.8 ± 0.7 mm	1.6 ± 0.6 mm

Fifty patients were scanned for at least 1 of the 4 measurement configurations. Values are mean \pm standard deviation. Reported values are the force measured by the load cell at the stabilized flow shear rate. The maximum velocity was measured by PIV (with the bracelet) or power Doppler (at natural flow). The estimated shear rate was obtained using Equation 2 for every vein diameter and maximum blood velocity (see Appendix 1). The coefficient of variation of the estimated shear rate corresponds to the standard deviation to mean ratio. The deepness and diameter of the vein were measured from B-mode images. The maximum blood velocity target was fixed at 1 mm / s when the flow was controlled with the bracelet.

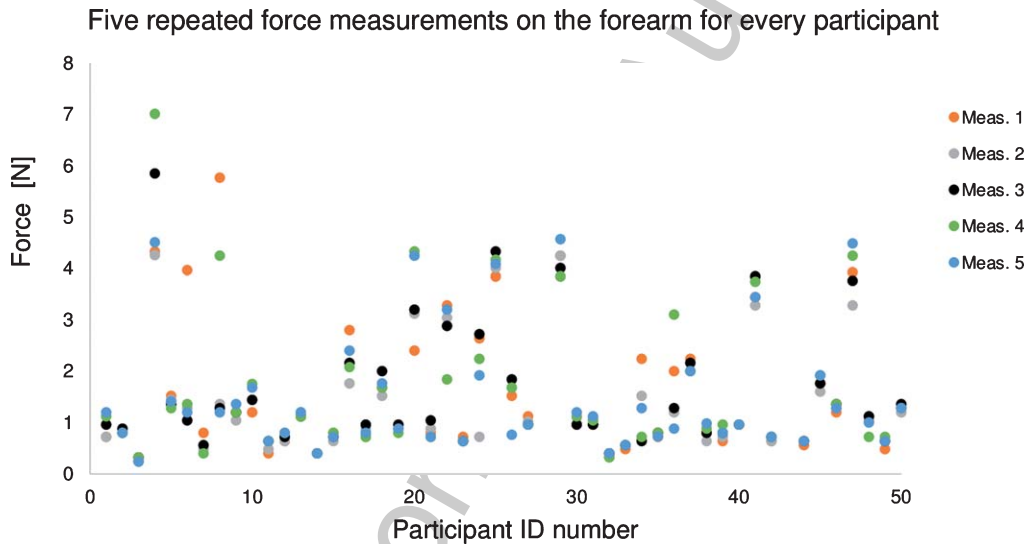


Fig. 4. Applied force required to reduce the blood flow within the vein to the targeted maximal blood velocity of 1 mm/sec for 5 repeated ultrasound measurements on the forearm of every participant. Participants #28 and #43 had no data for this configuration. The color of data points corresponds to the order in which measurements were taken. There was no association between the calibrated force applied on the skin and the measurement order (p -value >0.05 among 5 measurements).

variability of 16% and 17% on the forearm and leg, respectively). Between participants, the mean applied force varied from 0.3 to 5.2 N (inter-subject variability of 76% and 70% on the forearm and leg, respectively). For both venous sites, the patient age, vein's depth, and BMI were not correlated with the applied force required to control the flow. Measurements showed no trend between the force applied and the acquisition order (p -value >0.05) for both forearm and leg (*i.e.*, no memory effect).

Table 2

Comparison of SFSAE ultrasound parameters D and W measured on the forearm and leg at low and natural shear rates

SFSAE measurements	Forearm			Leg		
	N	SFSAE \pm SD	ICC [95% CI]	n	SFSAE \pm SD	ICC [95% CI]
D , low shear	48	1.46 \pm 0.35	0.84 [0.77, 0.90]	19	1.45 \pm 0.33	0.87 [0.77, 0.94]
W , low shear		5.46 \pm 2.73	0.77 [0.68, 0.85]		6.65 \pm 2.30	0.88 [0.79, 0.95]
D , natural shear	49	0.67 \pm 0.20	0.78 [0.69, 0.86]	36	0.66 \pm 0.18	0.81 [0.72, 0.88]
W , natural shear		1.39 \pm 0.70	0.66 [0.54, 0.77]		1.86 \pm 0.85	0.68 [0.56, 0.80]

Values are mean \pm standard deviation of 5 repeated ultrasound measurements for every configuration. The intraclass correlation coefficient (ICC) and its confidence interval are also presented. An ICC between 0.75 and 0.9 corresponds to a good reliability of the measurement. N : number of participants.

3.2. Ultrasound SFSAE aggregation measurements

The mean value, standard deviation and intraclass correlation coefficient (ICC) of D and W for all measurement configurations are shown in Table 2. When looking at averaged values of D or W , it can be noticed that they are similar for measurements on the arm or the leg. The same observation holds for the standard deviation and the intraclass correlation coefficient. As expected, both D and W showed higher values at low shear rate. In general, ICCs reveal better reliability for D than W . With ICC values higher than 0.75, measurements presented a good reliability except for W at natural shear rates, which presented moderate reliability. According to reported ICC values, the leg site seemed a better location for quantitative ultrasound aggregation measurements.

3.3. SFSAE repeatability

In the remaining of this manuscript, to simplify figure displays, only the SFSAE parameter D is reported (similar results were obtained for W). To illustrate all data points used to compute a single value in Table 2, all individual measurements of D at low shear rate on the forearm are displayed in Fig. 5. The mean value of D for this configuration was 1.46, with an intra-subject variability of 26.3%, ranging from 5.7% (participant #26) to 91.5% (participant #4). The color of data points corresponds to the order in which measurements were taken. Measurements showed no trend between data point values and their acquisition order in the sequence of 5 measures (p -values >0.05 for both forearm and leg configurations).

3.4. Relation between forearm and leg measurements

Measurements of D on the leg and on the forearm were correlated as displayed in Fig. 6 for both shear rate conditions. Low shear rate measurements spread well along the regression line (round blue dataset over the blue dotted line) with a coefficient of determination of 0.77. This strong relation is confirmed by the Spearman's correlation coefficient $\rho = 0.84$ (p -value <0.01). Results were similar for W at low shear rate ($\rho = 0.78$, p -value <0.01). At natural shear rate, less variation in RBC aggregation between individuals was noticed; measurements of D in Fig. 6 were packed close to the origin (orange diamond dataset). Correlation coefficients for D and W between the leg and the forearm at natural flow were the same at $\rho = 0.52$ (p -values <0.01).

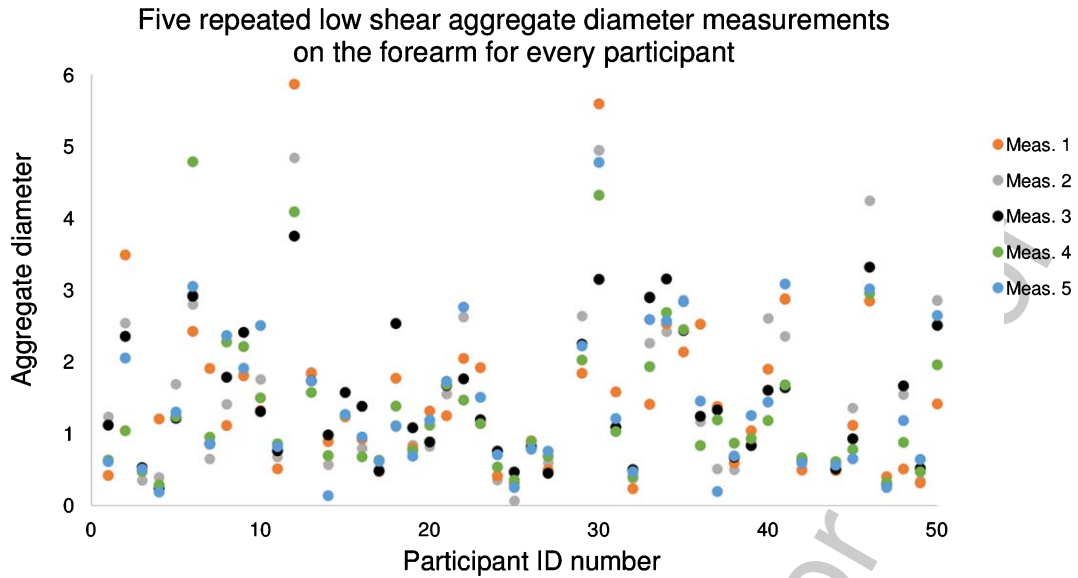


Fig. 5. Plot of 5 measured values of the ultrasound aggregation diameter (parameter D) on the forearm at a low shear rate for every participant. Participants #28 and #43 had no data for this configuration. The color of data points corresponds to the order in which measurements were taken. There was no association between the aggregate diameter and the measurement order (p -value >0.05 among 5 measurements).

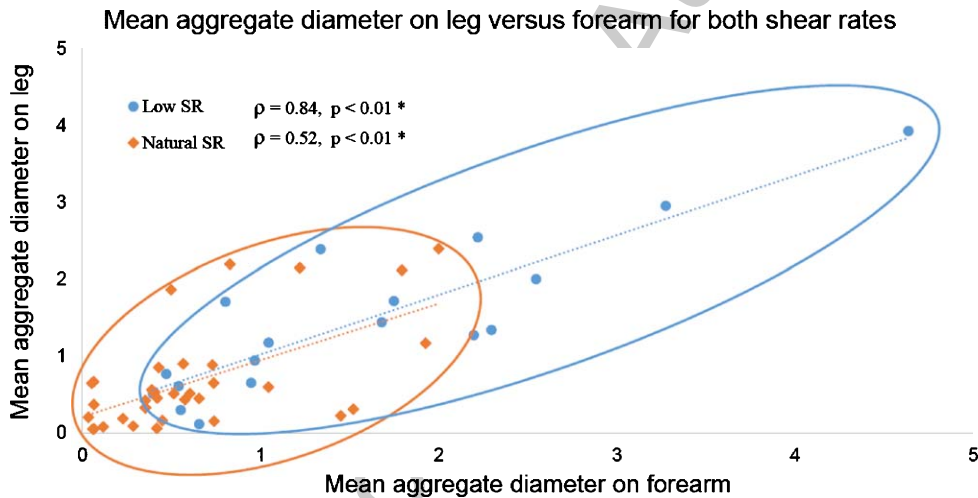


Fig. 6. Aggregate diameter (D parameter) on the forearm and leg are proportional for measurements at low shear (blue) and natural shear rate (orange) conditions. SR: shear rate.

3.5. Relation between natural and low shear rate measurement conditions

Figure 7 compares D values that were measured for each participant at natural and low shear rate conditions. Both forearm (black dot dataset) and leg (red diamond dataset) measurements are displayed on this figure and present similar trends. Similarities of measurements at both shear rates are confirmed by Spearman's correlation coefficients $\rho = 0.74$ (p -value <0.01) for the forearm, and $\rho = 0.56$ (p -value = 0.025) for the leg. With W , correlations were $\rho = 0.76\%$ (p -value <0.01) for the forearm, and

230

231

232

233

234

235

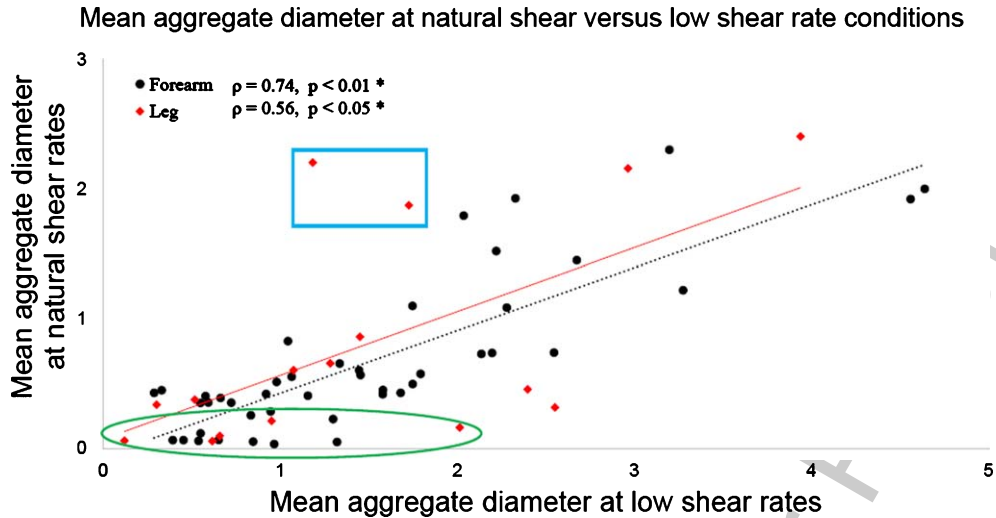


Fig. 7. SFSAE D parameter on both forearm and leg at natural shear rate versus low shear rate conditions. The low shear obtained by using the compression bracelet increased the range of D values for participants with naturally high venous flow (green ellipse), and contributed to standardise measurements for those with very low venous flow (blue box).

236 $\rho = 0.44$ (p -value = 0.090, non-significant) for the leg. As noticed in Fig. 7, some measurements were
 237 close to the abscissa, as highlighted by the green ellipse. For these participants, the natural blood veloc-
 238 ity measured by Doppler ultrasound was higher than for the other participants, on average 38 mm/s
 239 compared to 23 mm/s. For these individuals, the natural shear rate was too high to promote aggrega-
 240 tion. In these particular cases, D values given by the SFSAE method at natural shear was close to 0.1
 241 compared to 1.0 for measurements at low shear rate on the same participant. Above the regression
 242 line are two participants presenting high D values at natural shear and lower D at low shear rate, as
 243 highlighted by the blue box. The natural blood flow speed for these two participants was too small
 244 to be measured by Doppler ultrasound, whereas at reduced flow controlled by the bracelet the mean
 245 velocity measured by PIV was around 0.5 mm/s.

246 3.6. *Ex vivo* S_{10} versus SFSAE aggregation measurements

247 RBC aggregation measurements made on blood samples using the erythroaggregometer ranged from
 248 14.2 to 28.9 (21.6 ± 3.6). Since S_{10} and *in vivo* SFSAE parameters describe laser and ultrasound RBC
 249 aggregate backscattering properties, respectively, it was interesting to explore the relation between
 250 both approaches. Figure 8 presents D at low shear rate as a function of the *ex vivo* parameter S_{10} . One
 251 can notice that D tends to increase proportionally with S_{10} . Similar relations were noticed for D at
 252 natural flow and for W at both flow conditions (not shown). Significant correlation coefficients were
 253 measured between D or W assessed on the forearm at both shear rates and S_{10} ($0.64 < \rho < 0.72$, p -values
 254 < 0.01). SFSAE measurements on the leg at low shear rate condition were also correlated with S_{10} (for
 255 D : $\rho = 0.81$, p -value < 0.01 ; and for W : $\rho = 0.76$, p -value < 0.01). However, SFSAE measurements at
 256 natural flow on the leg were weakly correlated with S_{10} (for D : $\rho = 0.35$, p -value = 0.09, non-significant;
 257 and for W : $\rho = 0.34$, p -value = 0.04).

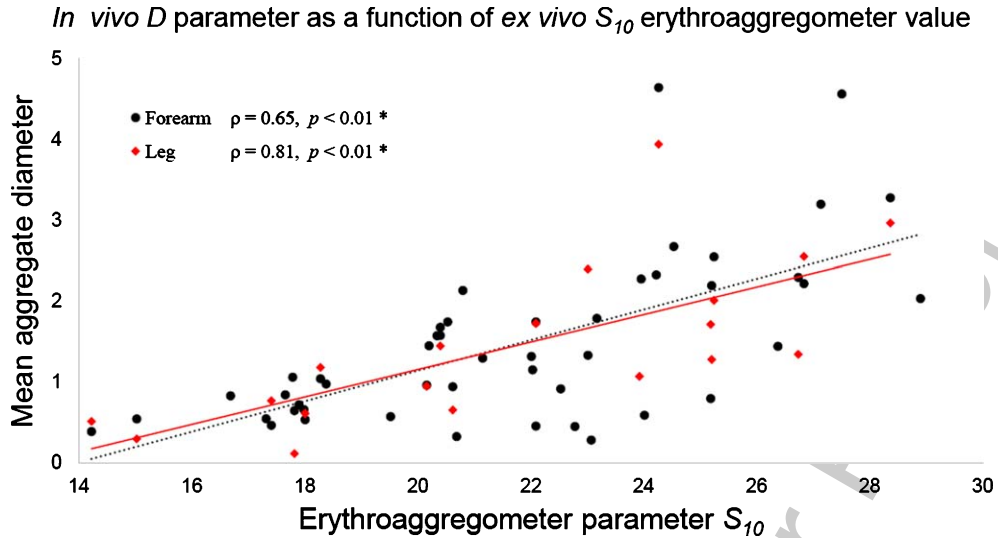


Fig. 8. SFSAE D parameter on both forearm and leg at low shear rates versus the *ex vivo* erythroaggregometer parameter S_{10} . D values increased proportionally with S_{10} , as shown by the linear fitting curve.

4. Discussion

Several contributions were made in this study. A computer interface was designed to monitor acquired RF data, to adjust the blood flow velocity to obtain the targeted low shear rate value, and to display in real-time the force applied by the pressurized bracelet on the vein. This is the first study to evaluate the repeatability of SFSAE parameters D and W . We could also establish that SFSAE measurements on the antebraial vein of the forearm or tibial vein of the leg provided similar assessment of the systemic level of RBC aggregation. Significant correlations could also be demonstrated between *in vivo* assessments of RBC aggregation and *ex vivo* laboratory measures of the aggregation kinetics.

4.1. Adjustment of the force applied to reduce the blood flow

As seen in Fig. 4, a wide range of applied pressure was required among participants to reduce the venous flow to the targeted value. Indeed, Garcia-Duitama et al. [14] proposed keeping the shear rate below 3 s^{-1} for obtaining measurements under stable aggregation conditions. However, as reported in Table 1, the shear rate at natural flow was on average 37 s^{-1} , approximately. Consequently, this means that without any flow control, the shear rate in the vein would be well above the proposed threshold for optimum measures. Also, as noticed in Fig. 7, two participants had natural flow close to stasis (blue box) and values of D (and W) higher than under the controlled flow condition. For these participants, the use of the bracelet was not helpful to control the blood flow. Thus, according to results of Figs 4 and 7, a standard pressure that would apply to all participants to reduce the blood flow could not be established. Also, as demonstrated by Garcia-Duitama et al. [14], assessing RBC aggregation under stasis condition could not be a solution. Indeed, this approach is not reproducible because the natural flow before stoppage would provide variable RBC aggregation states affecting the aggregation kinetics and ultrasound measurements.

As indicated in Table 1, standard deviations of the shear rate at natural flow were quite large, especially in lower limbs. Coefficients of variation of 59% and 102% at natural flow were reduced to 30% and 38% under controlled flow. Therefore, the bracelet was useful to avoid variable measurements

283 under natural flow due to the different states of RBC aggregation; see data in the green ellipse of Fig. 7.
284 By decreasing the shear rate, RBC aggregation was enhanced and better controlled, and a wider range
285 of D and W could be observed, reflecting different levels of aggregation. However, even if coefficients
286 of variation on reported shear rates were lower when the bracelet was used, corresponding ICCs with
287 the bracelet were 0.45 in the forearm and 0.49 in the leg, showing poor reliability of the shear rate
288 control. This suggests that the blood flow adjustment technique and device could be further improved.
289 An automatic control of the blood pressure applied by the bracelet through a feedback loop would
290 undoubtedly provide greater stability of the blood flow and better repeatability of the aggregation
291 measurement. In addition, because only 19 out of 50 measurements could be performed on the leg
292 site at low shear rate, this also supports the need of redesigning a new compression device. A rotating
293 bracelet with a different footprint coupled with a miniaturised transducer might be more adapted for
294 measurements over the leg (ankle).

295 4.2. Ultrasound SFSAE aggregation measurements

296 4.2.1. SFSAE robustness

297 The reliability of SFSAE parameters was tested using the intraclass correlation coefficient (ICC).
298 Results in Table 2 showed an overall good reliability for D and W . The best ICC scores were obtained
299 for low shear rate measurements with excellent values ranging from 0.77 to 0.88, thus showing the
300 relevance of controlling the blood flow. In general, ICCs indicated better reliability for D than W . The
301 relation $W \approx D^2$ between the two parameters leads to larger values and larger coefficients of variation
302 for W and therefore a lower robustness. This relation could also explain why D and W are correlated
303 together ($0.86 < \rho < 0.96$, p -values < 0.001) when considering all measurements, and thus reporting
304 figures on D 's results only was justified.

305 Baskurt et al. [23] already discussed the fact that the *in vivo* shear rate history could affect aggregation
306 measurements. With most erythroaggregometer laboratory instruments, a high shear rate is applied to
307 break RBC rouleaux and clumps before assessing the kinetics of aggregation. For *in vivo* assessments,
308 we previously concluded that maintaining a residual flow for a given period of time improved the
309 repeatability of ultrasound measurements of RBC aggregation [14]. To limit the memory effect (i.e.,
310 RBC aggregation depending on the shear rate history), a bracelet was designed to locally control the
311 blood flow in the vein; a cuff as used to measure blood pressure would not be adequate as it would
312 stop the flow in all peripheral veins of the limb. Also, in the current study, a one minute waiting period
313 was used to measure RBC aggregation after reducing the flow. Moreover, a one minute waiting at
314 natural flow was also allowed to let RBCs retrieve their natural aggregation state before taking another
315 measurement. It was interesting to notice from Fig. 5 that the waiting period of one minute between
316 measurements was sufficient to avoid any memory effect. Indeed, no trend was noticed between the
317 value of D and the order of measurements. The choice of large veins for measurements (mean diameters
318 between 1.43–1.82 mm, Table 1) likely contributed to the robustness of D and W because the natural
319 flow (around 28 mm / s, Table 1) seemed sufficient to return to the natural aggregation state within one
320 minute.

321 4.2.2. Relation between forearm and leg measurements

322 In the past, *in vivo* assessment of RBC aggregation with the ultrasound SFSAE method has been
323 conducted in diabetes mellitus patients with poor metabolic control (proof-of-concept study) [13].
324 Ultrasound measurements were performed within the cephalic vein in the proximal portion of the
325 forearm and the saphenous vein in the distal portion of the leg. Hyper aggregation was detected in
326 diabetic patients within both forearm and foot veins but correlation between measurements at both sites
327 was not assessed in that study. Results in Table 2 showed very similar values of both SFSAE parameters

328 between measurements in the forearm and the leg. This relation is confirmed by the correlation $\rho = 0.84$
329 for D (p -value < 0.0001) and $\rho = 0.75$ for W (p -value < 0.001) between measurements made at these
330 two sites with the bracelet. When measured at natural flow, the correlation for both parameters was
331 not as good but significant ($\rho = 0.52$, p -value $= 0.001$ for D ; and $\rho = 0.46$, p -value < 0.01 for W). We
332 can therefore consider ultrasonic assessment of erythrocyte aggregation as a systemic measure since
333 values taken at two distinct sites were highly correlated.

334 The idea of a systemic measurement of erythrocyte aggregation was already proposed by Kitamura
335 & Kawasaki [9]. As far as we know, this study was the first to present a systemic quantitative mea-
336 surement of RBC aggregation within a vein using ultrasound. However, their measurements remained
337 greatly influenced by the echogenicity of blood that was not assessed using the instrument independent
338 backscatter coefficient. The current SFSAE modeling was based on fitting the spectral content of the
339 backscatter coefficient. In the light of the present study, it is conceivable to provide to intensivists a
340 quantitative RBC aggregation measure that is related to systemic inflammation [1]. RBC aggregation
341 assessed by the proposed SFSAE model has also been shown to be a prognostic measure of venous
342 thrombosis [24]. A limitation of the current method based on high-frequency ultrasound imaging
343 (35 MHz) might be the difficulty of imaging deep vessels because ultrasound attenuation depends on
344 frequency. It is theoretically feasible to measure local differences in RBC aggregation, which would be
345 relevant to characterize diseases such as the diabetic foot syndrome, critical limb ischemia or gangrene
346 [25, 26] but measurements would be limited to superficial vessels (depth limited to a few mm at
347 35 MHz).

348 4.2.3. Relation between natural and low shear rate measurements

349 The impact of the shear rate on erythrocyte aggregation has long been described [27]. Cloutier &
350 Qin [28, 29] went one step further by demonstrating the relation between the shear rate and ultrasound
351 backscattering for various aggregating blood samples. A common technique to measure erythrocyte
352 aggregation *ex vivo* consists in controlling the shear rate in a mechanical set-up, such as a Couette
353 or a microfluidic device [23]. As discussed earlier, this is more challenging *in vivo* and the use of a
354 bracelet equipped with a pneumatic occluding device allowed obtaining reproducible results on RBC
355 aggregation. Measurements performed at a low shear rate allowed determining consistent aggregation
356 level for all participants.

357 As reported in Fig. 6 and as expected, the aggregate diameter was larger at low shear rate (blue circle
358 dataset) than at natural shear rate (orange diamond dataset). In Fig. 7, every participant, except the two
359 with data in the blue box discussed above, had an aggregate diameter close to twice bigger at low shear
360 than at natural shear. The data in the green ellipse revealed a large difference in aggregate diameters
361 at natural versus low shear rates. This could be explained by the presence of high venous blood flow
362 for these participants. Again, this is emphasizing the importance of reducing and controlling the blood
363 flow because otherwise it would not have been possible to identify the varying aggregation levels for
364 these participants. Interestingly in Fig. 6, natural and low shear rate measurements exhibited the same
365 trend between measurement sites (*i.e.*, a slope close to 1). This observation illustrates the consistency
366 of the proposed method despite the drastic difference in blood flow conditions, as the mean shear rate
367 was close to 50 times lower (Table 1) for measurements with bracelet than without.

368 The coefficient of variation, defined as the standard deviation to mean ratio, allows comparing
369 the variability of different measurement categories. Mean and standard deviation values reported in
370 Table 2 for SFSAE parameters gave higher variability at natural shear than at low shear. For example,
371 coefficients of variation for aggregate diameters measured at the forearm's site were 24% and 30%
372 at low and natural shear rates, respectively. Likewise, the coefficient of variation for the reference
373 aggregation measure S_{10} was 17%. The fact that the coefficient of variation was slightly larger for
374 ultrasound than *ex vivo* measurements illustrates the need for a good shear rate control device.

375 However, conditions of hyper-aggregation could reduce the importance of a precise shear rate control
376 on measurements since aggregates would be more shear rate resistant. Using *ex vivo* erythroaggre-
377 gometer, the strength of aggregates has been defined as the minimum shear rate threshold necessary
378 to partially dissociate RBC aggregates. Le Devehat et al. [30] measured increased partial dissociation
379 threshold (PDT) of 54.5 s^{-1} for diabetic patients with severe leg ischemia versus 47.0 s^{-1} for healthy
380 subjects. The same conclusion was reached by El Bouhmadi et al. [31] who found an increased PDT of
381 78.1 s^{-1} for women suffering from ovarian cancer versus 52.6 s^{-1} for women in the control group. Our
382 team using an ultrasound mean reported that a shear rate as high as 200 s^{-1} was necessary to break RBC
383 aggregates in patients with diabetes mellitus and poor metabolic control [32]. It is therefore possible
384 to hypothesize that in the context of hyper-aggregation, we may have a larger range of shear rates on
385 which the ultrasound assessment of RBC aggregation would be consistent.

386 4.3. *Ex vivo* S_{10} vs SFSAE aggregation measurements

387 When the blood flow was controlled with the bracelet, strong correlations were observed between D
388 and W parameters and the *ex vivo* S_{10} reference standard. This finding remained valid for measurements
389 on forearm's and leg's sites (Fig. 8). Consequently, as discussed above, ultrasonic measurements of
390 RBC aggregation can be seen as a local measure reflecting a systemic property. At the natural shear
391 rate, the same trend was observed on the forearm's site but not on the leg, where data showed weak
392 and non-significant correlations with S_{10} . In our cohort, $S_{10} = 21.6 \pm 3.6$, which is close to the value
393 of 23 ± 4 reported for healthy subjects [5].

394 4.4. Limitations

395 The sample size of this cohort was too small to study the influence of diseases, age, drugs, native
396 hematocrit or ethnicity on aggregation parameters D , W or S_{10} . However, Student t -tests showed
397 significant differences in D and W values between men and women. This difference in RBC aggregation
398 according to gender was already reported using *ex vivo* laser backscatter measurements [34]. On the
399 other hand, a relation between obesity and erythrocyte aggregation has also been described [35–37].
400 The current cohort was composed of healthy participants having a BMI around 25 and did not include
401 obese individuals. However, a significant correlation was nevertheless noticed between the BMI and
402 S_{10} ($\rho = 0.54$, p -value < 0.01), but not between BMI and SFSAE parameters.

403 Some limitations still hamper the immediate use of this technology for clinical diagnosis. The cur-
404 rent bulky ultrasound system may not be optimum for use in critical care or surgery units. A compact
405 ultrasound device would be more appropriate for these applications. Furthermore, acquisitions were
406 performed at 35 MHz, which is not a typical frequency used by clinical scanners that operate typically
407 between 3 to 15 MHz. Consequently, a dedicated portable miniaturized bed-site high-frequency ultra-
408 sound system would need to be developed. Such system would ideally include a monitor displaying
409 time-varying D and W parameters. Indeed, for monitoring RBC aggregation and thus systemic inflam-
410 mation, the specific value of a given parameter might be less crucial than its evolution over time under
411 similar flow conditions. From a clinical point of view, it is difficult to predict whether the venous flow
412 will remain constant throughout the aggregation monitoring procedure. This is why it seemed more
413 appropriate to control the venous flow and to adjust it at a very low shear for which RBC aggregation
414 is promoted in order to maintain a margin if the patient's condition deteriorates. It would eventually
415 be important to assess the day-to-day or week-to-week reproducibility of SFSAE measures. Thus to
416 summarize, challenges remain important but feasible.

5. Conclusions

Although the shear rate control may still require further improvements for *in vivo* measurements of erythrocyte aggregation, this study has demonstrated the feasibility of obtaining reproducible and non-invasive values in a clinical context. Structural parameters D and W describing RBC aggregation followed the same behavior at low and natural shear rate conditions, albeit values being higher at low shear rate. For monitoring RBC aggregation and thus systemic inflammation, the specific value of a given parameter might be less crucial than its evolution over time under similar flow conditions. From a clinical point of view, it is difficult to predict whether the venous flow will remain constant throughout the aggregation monitoring procedure. This is why it seemed more appropriate to control the venous flow and to adjust it at a very low shear for which RBC aggregation is promoted in order to maintain a margin if the patient's condition deteriorates.

In vivo results at low shear showed strong correlations between D and W , and the *ex vivo* S_{10} aggregation parameter, no matter the measurement site. For the detection of hyper-aggregation, standardized flow measurements might remain important to compare results from patient to patient, even though the confounding impact of the shear rate might be less critical. This study also showed that a bracelet equipped with a pressurized device was useful to control the blood flow and to obtain standardized *in vivo* measurement conditions. In routine clinical practice, the patient's forearm is often used for intravenous infusion of saline solution, vascular pressure monitoring, oxygen saturation measurements, etc . . . In this study, results obtained at leg's and forearm's sites were found to be correlated. Measurements followed the same tendency in both upper and lower limbs and this behavior was observed for both shear rates. The conceptualization of a new rotational bracelet design with a different footprint could allow optimizing measurements on patient's legs, which would facilitate monitoring in critical care units.

Acknowledgments

This study was financially supported by the Natural Sciences and Engineering Research Council of Canada (Collaborative Health Research Program #508337-17 and Engage Program #503381-16), and by the Canadian Institutes of Health Research (grant #CPG-151959). Authors want to thanks René Gosselin and Richard Côté from Menodys Inc. (Longueuil, Québec, Canada) for the helpful discussions, and every participants for their contribution to this pilot study.

References

- [1] Gyawali P, Ziegler D, Cailhier JF, Denault A, Cloutier G. Quantitative measurement of erythrocyte aggregation as a systemic inflammatory marker by ultrasound imaging: A systematic review. *Ultrasound in Medicine & Biology*. 2018;44(7):1303-17.
- [2] Urbach J, Shapira I, Branski D, Berliner S. Acute phase response in the diagnosis of bacterial infections in children. *The Pediatric Infectious Disease Journal*. 2004;23(2):159-60.
- [3] Imaizumi K, Shiga T. Effect of immunoglobulins and IgG-fragments on the human erythrocyte aggregation studied by a rheoscope combined with image analyzer. *Biorheology*. 1983;20(5):569-77.
- [4] Rampling MW, Whittingstall P, Linderkamp O. The effects of fibrinogen and its plasmin degradation products on the rheology of erythrocyte suspensions. *Clinical Hemorheology and Microcirculation*. 1984;4(6):533-43.
- [5] Weng X, Cloutier G, Beaulieu R, Roederer GO. Influence of acute-phase proteins on erythrocyte aggregation. *American Journal of Physiology-Heart and Circulatory Physiology*. 1996;271(6):H2346-52.
- [6] Boynard M, Lelievre JC, Guillet R. Aggregation of red blood cells studied by ultrasound backscattering. *Biorheology*. 1987;24(5):451-61.

- 460 [7] Sigel B, Machi J, Beitler JC, Justin JR, Coelho JC. Variable ultrasound echogenicity in flowing blood. *Science*.
461 1982;218(4579):1321-3.
- 462 [8] Yuan Y, Shung K. Ultrasonic backscatter from flowing whole blood. I: Dependence on shear rate and hematocrit. *J*
463 *Acoust Soc Am*. 1988;84:52-8.
- 464 [9] Kitamura H, Kawasaki S. Detection and clinical significance of red cell aggregation in the human subcutaneous vein
465 using a high-frequency transducer (10MHz): A preliminary report. *Ultrasound in Medicine and Biology*. 1997;23(6):933-
466 8.
- 467 [10] Mamou J, Oelze ML. (Eds.), *Quantitative Ultrasound in Soft Tissues*, Heidelberg: Springer, 2013, p. 226.
- 468 [11] Franceschini E, Yu FT, Cloutier G. Simultaneous estimation of attenuation and structure parameters of aggregated red
469 blood cells from backscatter measurements. *The Journal of the Acoustical Society of America*. 2008;123(4):EL85-91.
- 470 [12] Yu FT, Cloutier G. Experimental ultrasound characterization of red blood cell aggregation using the structure factor
471 size estimator. *The Journal of the Acoustical Society of America*. 2007;122(1):645-56.
- 472 [13] Tripette J, Nguyen LC, Allard L, Robillard P, Soulez G, Cloutier G. In vivo venous assessment of red blood cell
473 aggregate sizes in diabetic patients with a quantitative cellular ultrasound imaging method: Proof of concept. *PLoS One*.
474 2015;10(4):e0124712.
- 475 [14] Garcia-Duitama J, Chayer B, Garcia D, Goussard Y, Cloutier G. Protocol for robust *in vivo* measurements of erythrocyte
476 aggregation using ultrasound spectroscopy. *Ultrasound in Medicine & Biology*. 2017;43(12):2871-81.
- 477 [15] Garcia D. A fast all-in-one method for automated post-processing of PIV data. *Experiments in Fluids*. 2011;50(5):1247-
478 59.
- 479 [16] Franceschini E, Yu FT, Destremes F, Cloutier G. Ultrasound characterization of red blood cell aggregation with inter-
480 vening attenuating tissue-mimicking phantoms. *The Journal of the Acoustical Society of America*. 2010;127(2):1104-15.
- 481 [17] Wang SH, Shung KK. An approach for measuring ultrasonic backscattering from biological tissues with focused
482 transducers. *IEEE Transactions on Biomedical Engineering*. 1997;44(7):549-54.
- 483 [18] Saha RK, Franceschini E, Cloutier G. Assessment of accuracy of the structure-factor-size-estimator method in deter-
484 mining red blood cell aggregate size from ultrasound spectral backscatter coefficient. *The Journal of the Acoustical*
485 *Society of America*. 2011;129(4):2269-77.
- 486 [19] Oelze ML, O'Brien Jr WD. Application of three scattering models to characterization of solid tumors in mice. *Ultrasonic*
487 *Imaging*. 2006;28(2):83-96.
- 488 [20] Donner M, Siadat M, Stoltz JF. Erythrocyte aggregation: Approach by light scattering determination. *Biorheology*.
489 1988;25(1-2):367-76.
- 490 [21] Koo TK, Li MY. A guideline of selecting and reporting intraclass correlation coefficients for reliability research. *Journal*
491 *of Chiropractic Medicine*. 2016;15(2):155-63.
- 492 [22] Ostwald W. Ueber die rechnerische Darstellung des Strukturgebietes der Viskosität. *Colloid & Polymer Science*.
493 1929;47(2):176-87.
- 494 [23] Baskurt O, Boynard M, Cokelet G, Connes P, Cooke BM, Forconi S, Liao F, Hardeman MR, Jung F, Meiselman HJ, Nash
495 G, Nemeth N, Neu B, Sandhagen B, Shin S, Thurston G, Wautier JL. New guidelines for hemorheological laboratory
496 techniques. *Clinical Hemorheology and Microcirculation*. 2009;42(2):75-97.
- 497 [24] Yu FTH, Armstrong JK, Tripette J, Meiselman HJ, Cloutier G. A local increase in red blood cell aggregation can trigger
498 deep vein thrombosis: Evidence based on quantitative cellular ultrasound imaging. *J Thrombosis & Haemostasis*.
499 2011;9:481-8.
- 500 [25] Khodabandehlou T, Vimeux M, Dévéhat CL. Measurements of transcutaneous oxygen pressure and changes in blood
501 rheology as markers of prognosis of critically ischemic limb in diabetes mellitus patients. *The International Journal of*
502 *Lower Extremity Wounds*. 2003;2(1):13-8.
- 503 [26] Mantskava M, Momtselidze N, Pargalava N, Mehedlishvili G. Hemorheological disorders in patients with type 1 or 2
504 diabetes mellitus and foot gangrene. *Clinical Hemorheology and Microcirculation*. 2006;35(1, 2):307-10.
- 505 [27] Schmid-Schönbein H, Gaetgens P, Hirsch H. On the shear rate dependence of red cell aggregation *in vitro*. *The Journal*
506 *of Clinical Investigation*. 1968;47(6):1447-54.
- 507 [28] Cloutier G, Qin Z. Ultrasound backscattering from non-aggregating and aggregating erythrocytes - A review. *Biorhe-*
508 *ology*. 1997;34(6):443-70.
- 509 [29] Cloutier G, Qin Z. Shear rate dependence of ultrasound backscattering from blood samples characterized by different
510 levels of erythrocyte aggregation. *Annals of Biomedical Engineering*. 2000;28(4):399-407.
- 511 [30] Le Devehat C, Khodabandehlou T, Vimeux M. Impaired hemorheological properties in diabetic patients with lower
512 limb arterial ischaemia. *Clinical Hemorheology and Microcirculation*. 2001;25(2):43-8.
- 513 [31] El Bouhmedi A, Laffargue F, Brun JF. Aggregability and disaggregability of erythrocytes in women suffering from
514 ovarian cancer: Evidence for an increased disaggregation threshold. *Clinical Hemorheology and Microcirculation*.
515 2000;22(2):91-7.

- 516 [32] Cloutier G, Zimmer A, Yu F, Chiasson JL. Increased shear rate resistance and fastest kinetics of erythrocyte aggregation
517 in diabetes measured with ultrasound. *Diabetes Care*. 2008;31(7):1400-2.
- 518 [33] Weng X, Cloutier G, Pibarot P, Durand LG. Comparison and simulation of different levels of erythrocyte aggregation
519 with pig, horse, sheep, calf, and normal human blood. *Biorheology*. 1996;33(4 & 5):365-77.
- 520 [34] Pignon B, Adjizian JC, Donner M, Stoltz JF, Potron G. Mesure de l'agrégation érythrocytaire par rétrodiffusion laser.
521 Détermination des valeurs normales. Influence de différents facteurs. In *Hémorhéologie et Agrégation Érythrocytaire.*
522 *Théorie et Applications Cliniques*. Cachan, Édition Médicales Internationales, France, Vol. 3, 1991, pp. 53-64.
- 523 [35] Guiraudou M, Varlet-Marie E, Raynaud de Mauverger E, Brun JF. Obesity-related increase in whole blood viscosity
524 includes different profiles according to fat localization. *Clinical Hemorheology and Microcirculation*. 2013;55(1):63-73.
- 525 [36] Solá E, Vayá A, Corella D, Santaolaria ML, Espana F, Estellés A, Hernández-Mijares A. Erythrocyte hyperaggregation
526 in obesity: Determining factors and weight loss influence. *Obesity*. 2007;15(8):2128-34.
- 527 [37] Samocha-Bonet D, Lichtenberg D, Tomer A, Deutsch V, Mardi T, Goldin Y, Abu-Abeid S, Shenkerman G, Patshornik H,
528 Shapira I, Berliner S. Enhanced erythrocyte adhesiveness/aggregation in obesity corresponds to low-grade inflammation.
529 *Obesity Research*. 2003;11(3):403-7.

530 Appendix 1: *In vivo* median shear rate estimation

The median shear rate can be conveniently approximated when the maximum blood velocity is known. To better approximate the blunted velocity profile characteristic of a non-Newtonian fluid such as blood, the blood viscosity was measured in a low shear viscometer (ProRheo LS300, Althengstett, Germany) over a range of shear rates varying from 0.5 to 100 s⁻¹. The blood kinematic viscosity, μ , was then fitted by least squares to the classical power law of Ostwald-De Waele [22]

$$\mu(\gamma) = a \cdot (-\gamma)^{b+1}, \quad (1)$$

where γ is the shear rate, and a and b are approximating coefficients. Then, by considering the vein as cylindrical and the flow as steady, and by applying the Navier-Stokes equation, the shear rate at a specific radial position, r , was estimated using

$$\gamma(r) = \left(-\frac{1}{2a} r \partial_z P \right)^{\frac{1}{b+1}}, \quad (2)$$

where $\partial_z P$ is the pressure partial derivative with respect to depth, defined as

$$\partial_z P = -2a \cdot \left(\frac{Q \cdot (3b + 4)}{\pi(b + 1)r^{\frac{3b+4}{b+1}}} \right)^{b+1}. \quad (3)$$

In Equation 3, Q corresponds to the volumetric blood flow, defined as a function of the maximum flow speed, v_{\max} , occurring at the central axis of vein, as

$$Q = \pi \cdot v_{\max} \cdot r^2 \cdot \frac{b + 2}{3b + 4}. \quad (4)$$

531 We used porcine blood experiments to approximate coefficients a and b : $a = 17.52 \pm 4.88$ and
532 $b = -0.33 \pm 0.07$. This was justified by the fact that porcine RBC aggregation is close to that of normal
533 human blood [33]. Using Equation 2 and establishing a shear rate threshold at 3 s⁻¹, we could verify
534 in Fig. 9 that all median shear rates for reported antebrachial experiments were below that threshold.
535 The targeted region corresponds to the red trapezoid in Fig. 9 where the y-axis indicates the measured
536 vein radius and the x-axis is the maximum velocity. A plot similar to Fig. 9 was used for tibial mea-
537 surements. Note that for a median shear rate under the threshold value of 3 s⁻¹, the relation between
538 v_{\max} and the vein radius corresponds approximately to $v_{\max} \leq 4 \times r$.

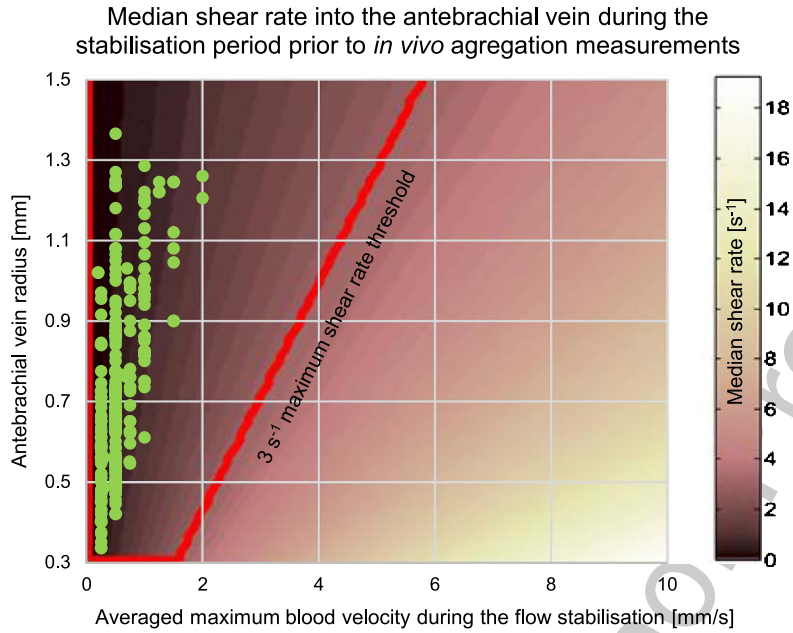


Fig. 9. Median shear rate in tube flow. The radius corresponds to the size of the antebrachial vein. The red box indicates the region for which the shear rate was less than $3 s^{-1}$. Green dots show estimated shear rates for every measurements made with the bracelet on the forearm.